



HZCS-III



—

—

—





$\geq 3KW$



HZCS-III

()

45H 55Hz

●

●

●

●

赫兹电力
HERTZ POWER

220V

380V

30A

1

45Hz


55Hz

225

027-83267669




-
-
-
-
-

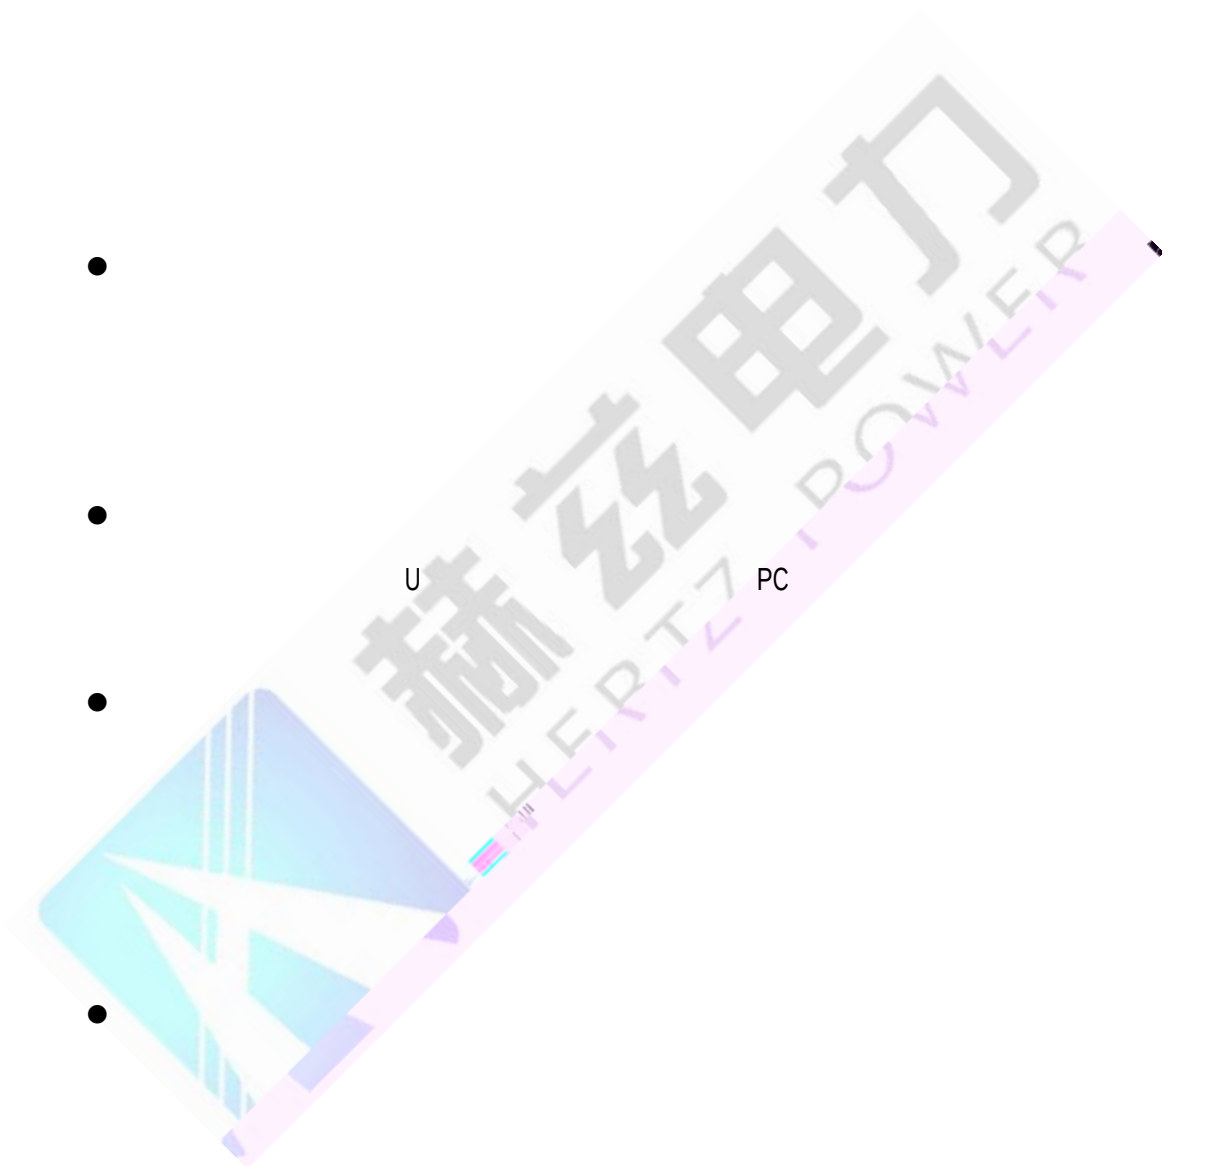

1		-20 50	RH 80%
2			
3		AC 220V ± 10%	3KW



4			AC250V
			0.5%
			0.5%
			8A
			45Hz 55Hz
5			0.01 30μF
			0.01 400Ω
			-180 ° +180 °
6			0.0001μF
			0.0001Ω
			0.0001 °
7		≥ 1μF ± 1%	± 0.01μF
		1μF ± 2%	± 0.01μF
		≥ 1Ω ± 1%	± 0.01Ω
		1Ω ± 2%	± 0.01Ω
		± 0.2 ° (1.0V	
		± 0.3 ° (:0.2V 1.0V)	
8		30A	
9		10KV	
10		550 L × 430 W × 530 H	
11		200 U	
12		67 Kg	

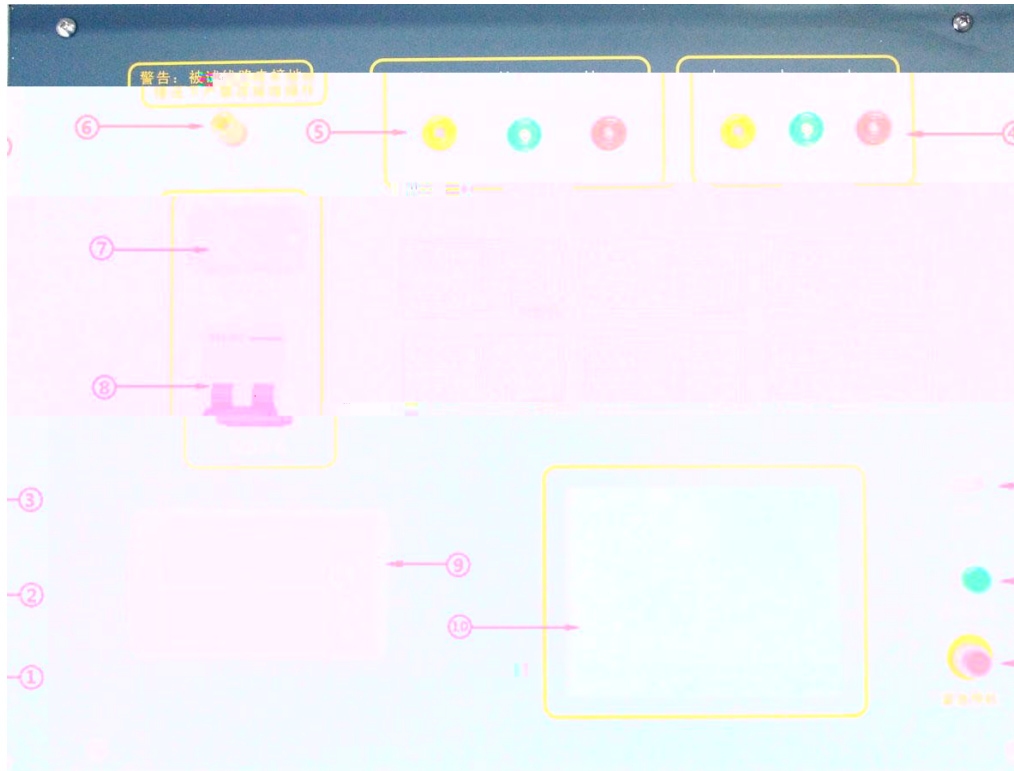

3-1

1

2

3

4

5

6

7

8

9

10

A

A

A 220

3.1

3—1—Φ



3.2

3—1—2

3.3 USB

3—1—3

U

U

USB

U

U

3.4

A B C

3—1—4

A

B

C

3

3.5

UA UB UC

3—1—5

UA

UB

UC

3

3.6

3—1—6

3.7

AC220V

3—1—7

225

027-83267669



3.8

3—1—⑧

3.9

3—1—⑨

55mm

3.10

$T = 10f \frac{1}{4}$
•
3—1—10

= 6

t






4—3

4

—4

10

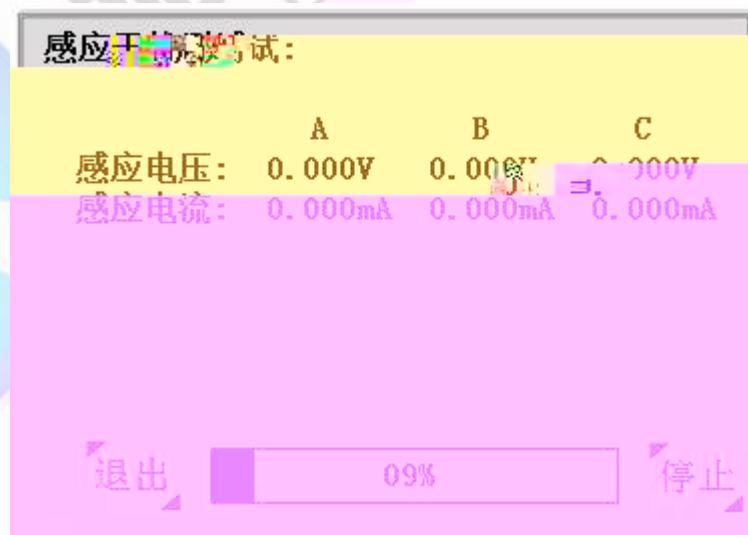

4—4

45Hz

200

4

200

4

45Hz

4—5

4—8

45Hz

55Hz

55Hz

4—6


4—9




,
4—6

4—7 4—10


4—4 4—5

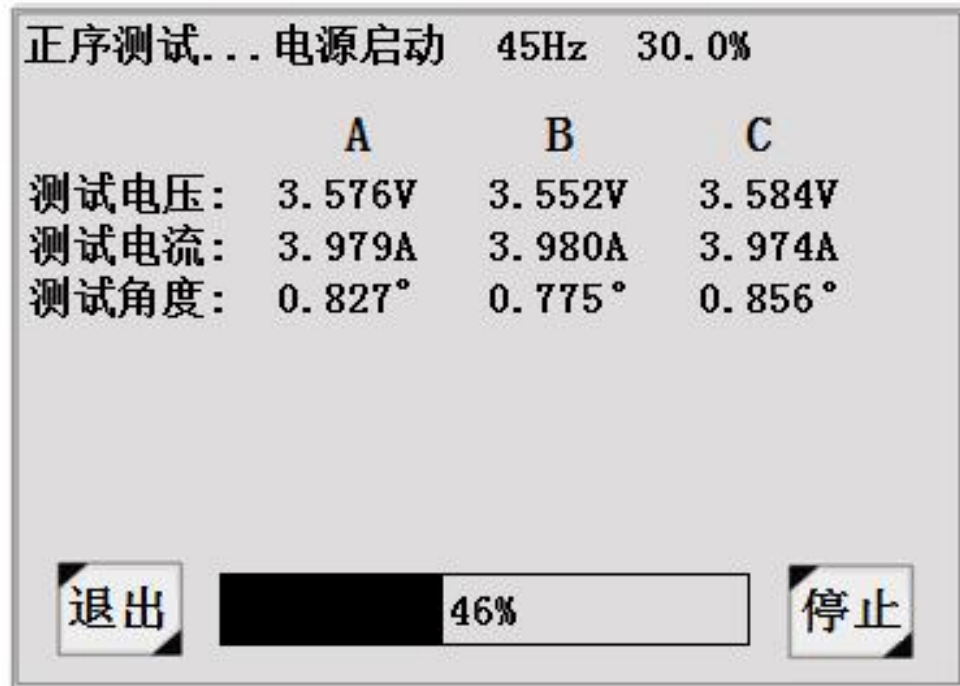


4—5

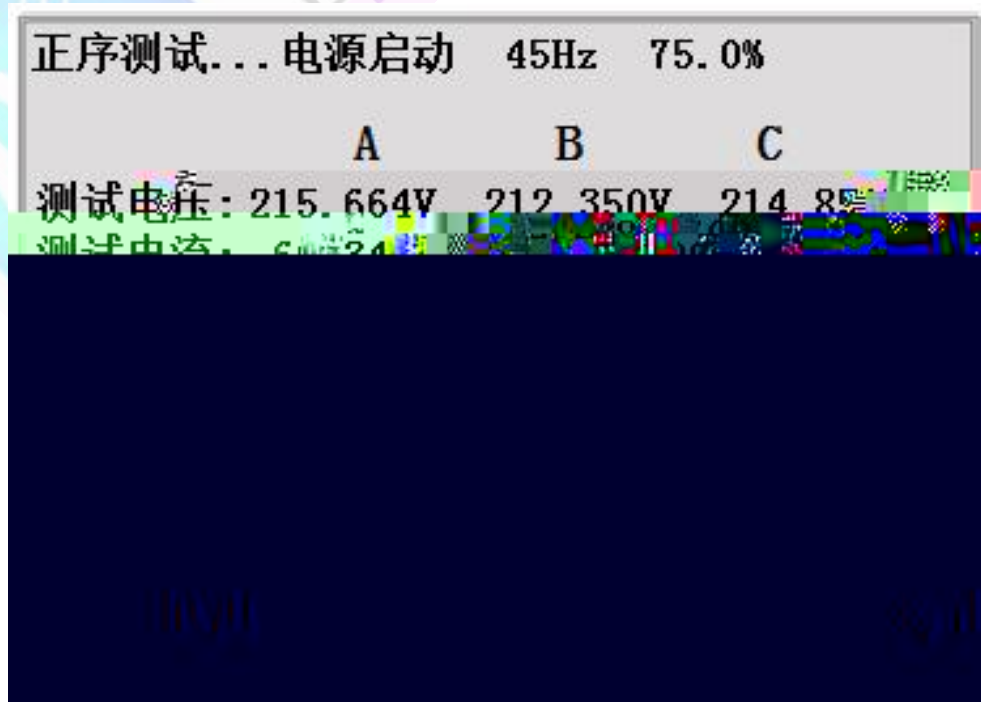

4—6

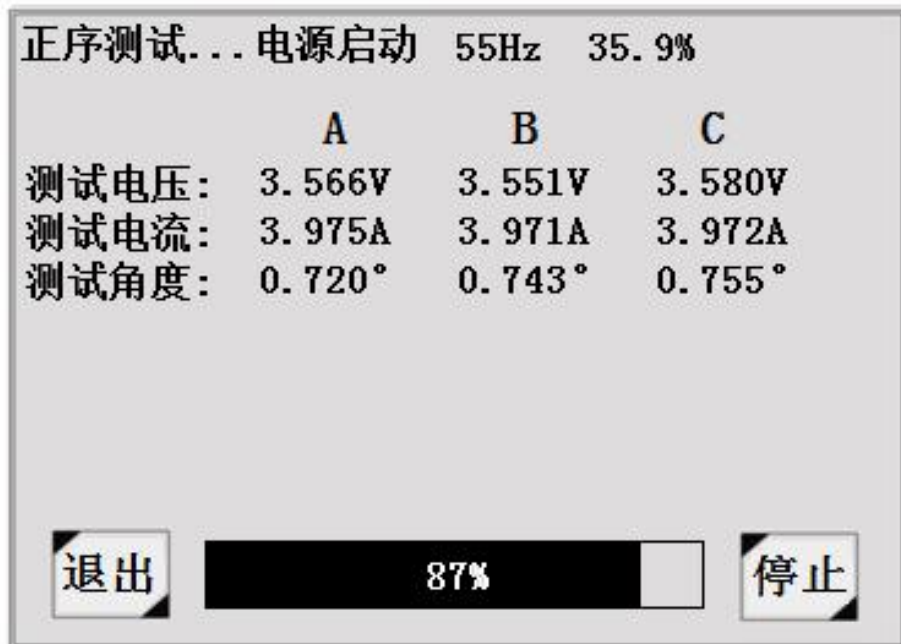

4—7

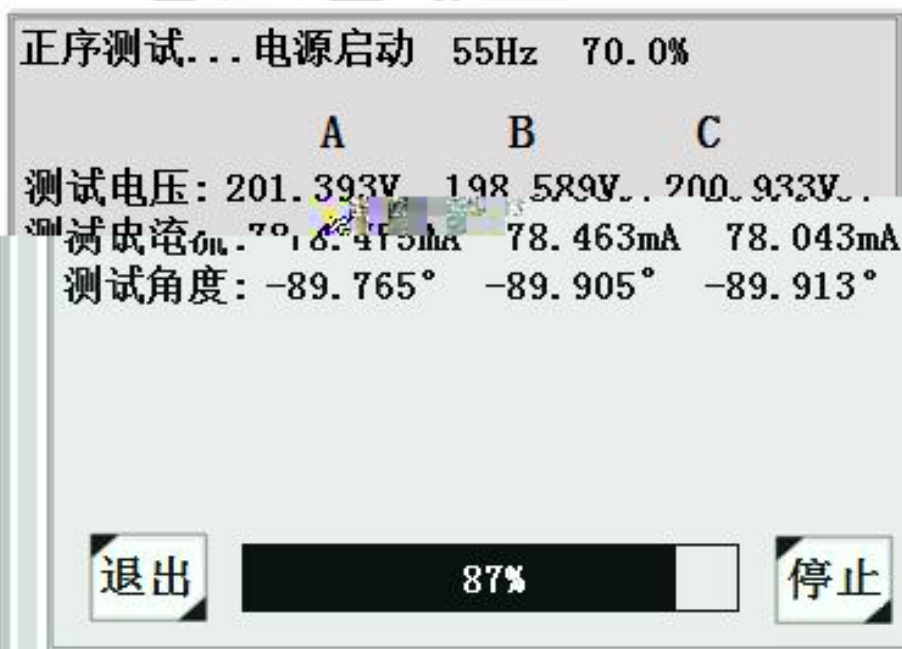

55



Z1 V :
R1 I :
X1 Φ :
Y1 Km:
G1
B1 :
C1 :

4—8

B

4.4

“ ”

4—11

4



4—11



4.5

“ ”

4—12

“ ”

4—13



4—12

日期	时间	长度	项目
00	2018-10-20 10:28	10.0	Z0
01	2018-10-20 10:24	10.0	Z1
02	2018-10-20 10:19	10.0	Z1
03	2018-10-20 10:13	10.0	Z1
04	2018-10-20 10:06	10.0	C1
05	2018-10-20 09:59	10.0	C0
06	2018-10-20 09:47	10.0	Zm
07	2018-10-20 09:41	10.0	C1
08	2018-10-20 09:33	10.0	C0
09			

退出

4—13




“ ” 4—12 “ U ”

U 4—14

4—14

“

”

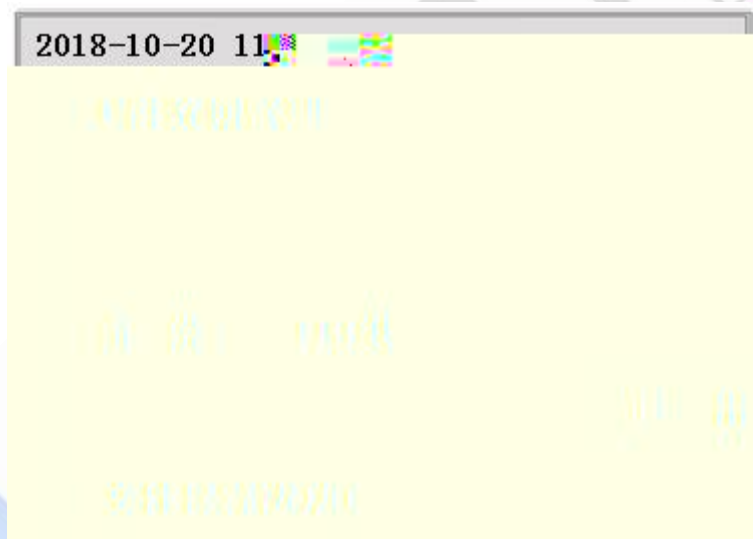

—

U

TXT

4.6

“ ”

4—15




4—15

IA IB IC ()


UA UB UC ()

5.1

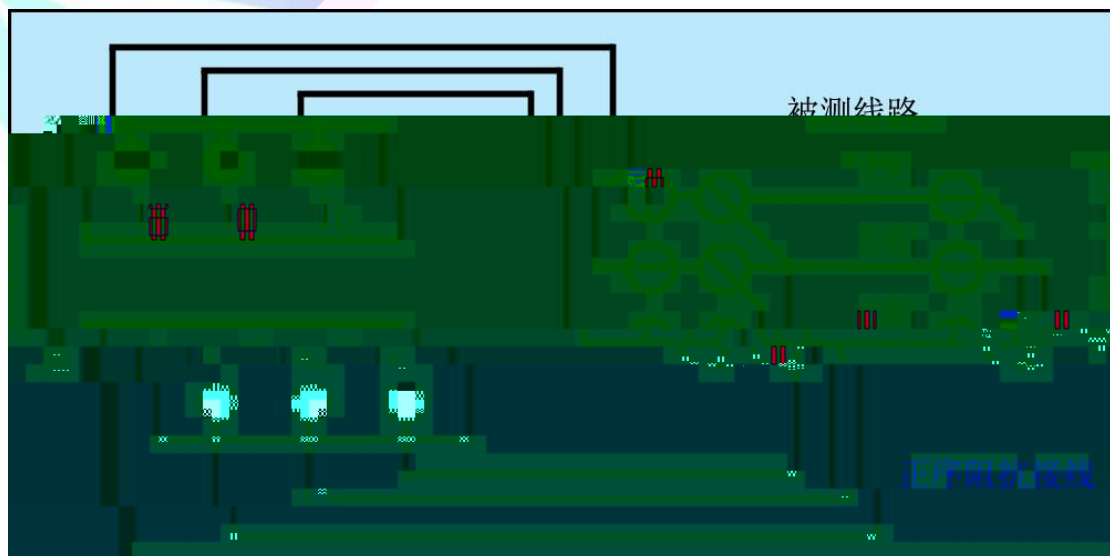


5—1

5.2

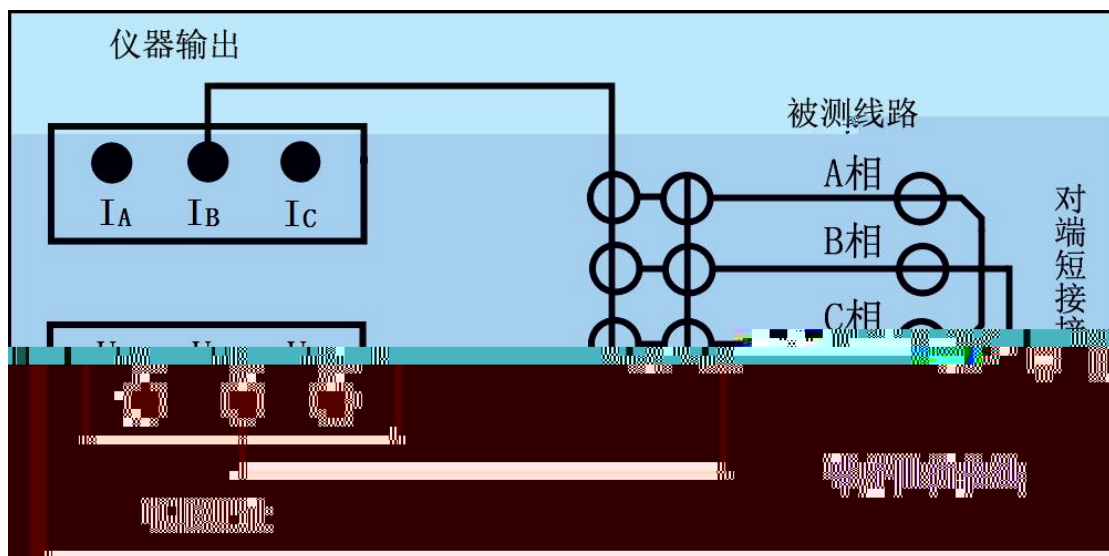


5—2

5.3

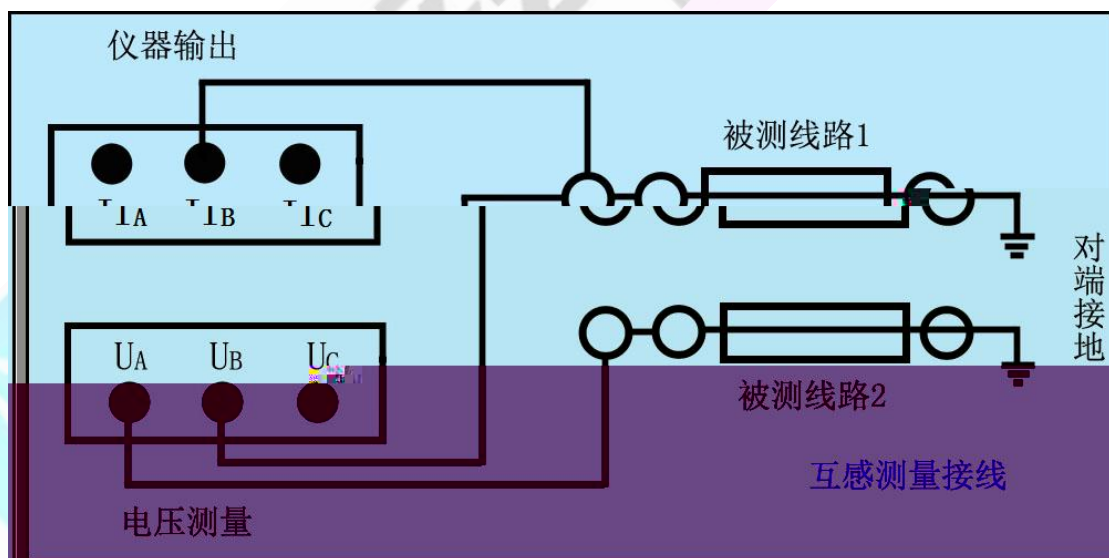


5—3

5.4

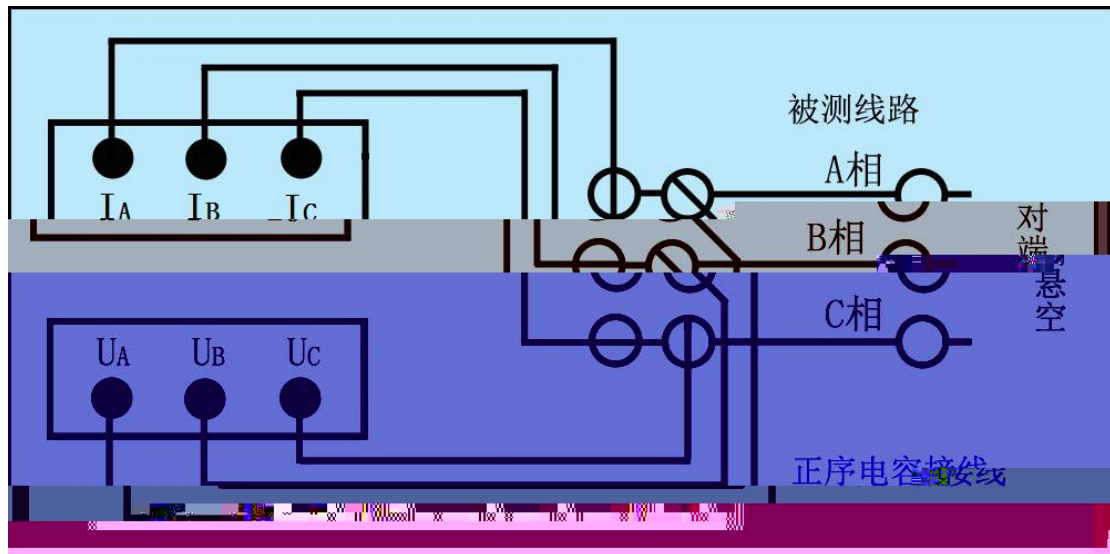


5—4

5.5

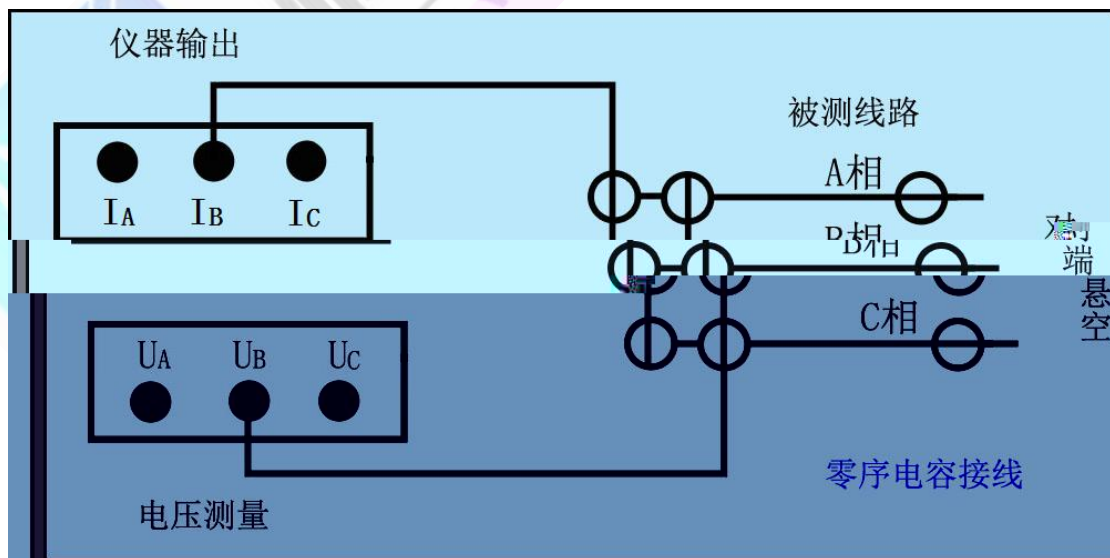


5—5

5.6

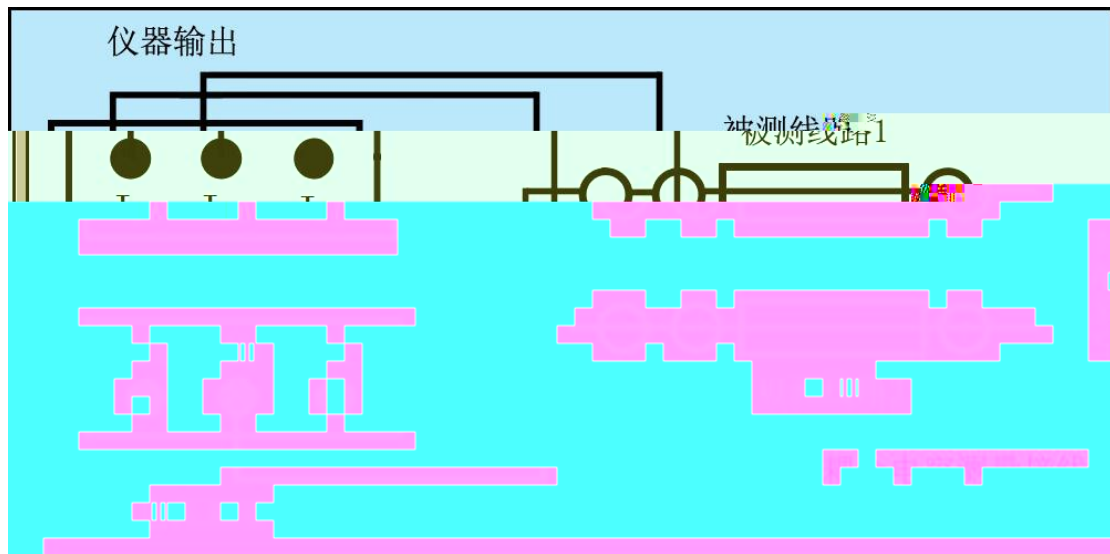

5—6

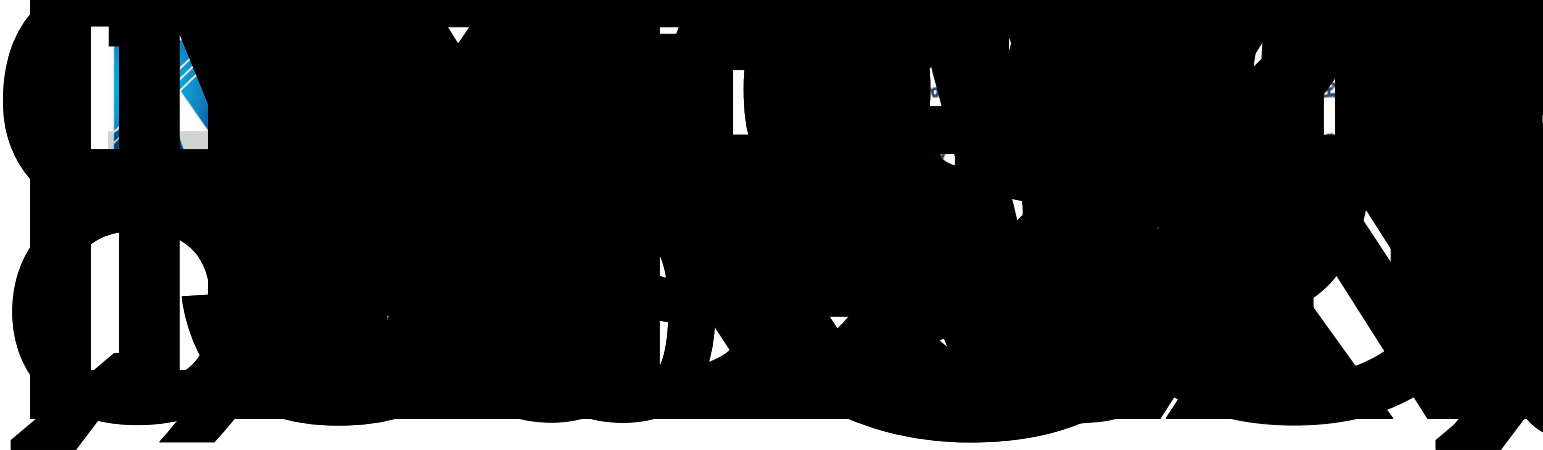

1

2 2010年10月10日

2010年10月10日

2

1 r

